



## Chicken IgY (IgG) ELISA

Catalog Number: 0801010

### INTENDED USE

Chicken IgY is the designation for the IgG-like molecule found in avian species. The IMMUNOtek Chicken IgY (IgG) ELISA is a rapid, easy to use enzyme linked immunosorbent assay (ELISA) designed for the measurement of chicken IgY in chicken serum, egg yolk or white, plasma, saliva, mucosa, cell culture fluid from chicken cells or other biological samples.

**The IMMUNOtek Chicken IgY (IgG) ELISA is for Research Purposes Only.**

### PRINCIPLE OF THE TEST

Microplate wells coated with polyclonal antibodies reactive to Chicken IgY form the capture phase of the assay. Chicken IgY specimen samples along with the supplied standard are diluted appropriately with Assay Diluent and are then incubated in the microplate wells. After a wash step, captured chicken IgY in the well is incubated with detector antibody, a polyclonal anti-chicken IgY conjugated to horseradish peroxidase (HRP). This antibody reacts only to the Fc portion of the immunoglobulin molecule allowing for the specific detection of IgY immunoglobulins. After another wash step, the chromogenic substrate tetramethyl benzidine (TMB) is added and a blue color develops in proportion to the amount of chicken IgY that has been bound to the antibody-coated plate. The enzyme reaction is stopped by the addition of Stop Solution which results in a color change to yellow that can be measured spectrophotometrically at 450 nm. The concentrations of chicken IgY are then calculated from a standard curve.

### REAGENTS

#### Materials Supplied:

- **Microplate, (1 x 96 well):** 12 x 8-well strips coated with goat anti-chicken IgY
- **Chicken IgY Detector Antibody (12 ml):** Contains HRP conjugated goat anti-chicken IgY (Fc fragment specific)
- **Chicken IgY Standard (7 ml):** Contains 125 ng/ml of chicken IgY in Assay Diluent
- **Assay Diluent (100 ml):** Contains PBS, blocking proteins, Triton X-100® and 2-chloroacetamide as a preservative.
- **10X Plate Wash Buffer (125 ml):** Contains PBS, Tween 20® and 2-chloroacetamide as a preservative
- **Substrate (12 ml):** Contains Tetramethyl Benzidine (TMB)
- **Stop Solution (12 ml):** Proprietary formulation
- **Microplate Sealers (1 pk):** 10 sealers per pack
- **Sealable Plastic Bag (1 bag):** For storage of unused microplate strips

Triton X-100 is a registered trademark of Dow Chemical Company.  
Tween 20 is a registered trademark of ICI Americas, Inc.

This product was manufactured in a facility which has a Quality Management System that is ISO 13485 certified.

REF	Catalog Number	↓	Temperature Limitation
LOT	Lot Number	↓	Expiration Date
RUO	For Research Use Only		

**ZeptoMetrix Corporation**  
878 Main Street  
Buffalo, NY 14202  
800-274-5487  
[www.zeptometrix.com](http://www.zeptometrix.com)



## Chicken IgY (IgG) ELISA

Catalog Number: 0801010

### Materials required but not supplied:

- Personal protection equipment (Disposable gloves, lab coat, safety glasses, etc.)
- Distilled or deionized water
- Graduated cylinders and beakers
- Test tubes and racks for preparing specimen and IgG standard dilutions
- Validated adjustable micropipettes and tips, single and/or multi-channel
- Timer
- Validated incubator or temperature controlled room at 18-25°C
- Absorbent paper towels
- Validated microplate reader capable of measuring optical density at 450nm
- Automatic microplate washer or manual vacuum aspiration equipment
- Graph paper or computer graphing software

### STORAGE

Store all kit reagents at 2-8°C. Do not freeze. Unused microplate strips should be kept in a sealed bag with desiccant to minimize exposure to moisture. All reagents stored and handled properly are stable at least until the expiration date printed on the kit box label.

### PRECAUTIONS

- Prior to performing the assay, carefully read all instructions.
- Use universal precautions when handling kit components and test specimens.\*\*
- To avoid cross-contamination, use separate pipette tips for each specimen.
- When testing potentially infectious specimens, adhere to all applicable local, state and federal regulations regarding the disposal of biohazardous materials.
- Stop Solution contains hydrochloric acid, which may cause severe burns. In case of contact with eyes or skin, rinse immediately with water and seek medical assistance. Wear protective clothing and eyewear.



\*\*MMWR, June 24, 1988, Vol. 37, No. 24, pp. 377-382, 387-388

### PREPARATION OF REAGENTS

#### Plate Wash Buffer:

Dilute 10X Plate Wash Buffer 1:10 in distilled or deionized water prior to use. Mix thoroughly. Prepared 1X Plate Wash Buffer can be stored at 2-8°C for up to one week. Additional 10X Plate Wash Buffer (ZMC Catalog #: 0801060) may be ordered if needed.

This product was manufactured in a facility which has a Quality Management System that is ISO 13485 certified.

REF	Catalog Number		Temperature Limitation
LOT	Lot Number		Expiration Date
RUO	For Research Use Only		

ZeptoMetrix Corporation  
878 Main Street  
Buffalo, NY 14202  
800-274-5487  
www.zeptometrix.com

## Chicken IgY (IgG) ELISA

Catalog Number: 0801010

### Chicken IgY Standard Curve:

The Chicken IgY Standard is provided at 125 ng/ml and should be diluted in Assay Diluent to prepare a standard curve as shown in the table below.

Tube Number	Concentration of Chicken IgY	Volume of Chicken IgY Standard	Volume of Assay Diluent
1	125 ng/ml	1000 $\mu$ l	0 $\mu$ l
2	62.5 ng/ml	500 $\mu$ l of #1	500 $\mu$ l
3	31.25 ng/ml	500 $\mu$ l of #2	500 $\mu$ l
4	15.6 ng/ml	500 $\mu$ l of #3	500 $\mu$ l
5	7.8 ng/ml	500 $\mu$ l of #4	500 $\mu$ l
6	0 ng/ml	0 $\mu$ l	500 $\mu$ l

### Specimen Dilutions:

Chicken serum or plasma is estimated to have ~7 mg/ml of IgY. Chicken egg yolks have about 6-13 mg/ml of IgY. Because of this, we recommend preparing a 1:250,000-300,000-fold dilution in Assay Diluent for initial testing. To reduce dilution error, three dilution steps are recommended. For example, three 1:65-fold serial dilutions, where 10 $\mu$ l is added to 640 $\mu$ l of Assay Diluent, is a convenient dilution scheme. Other specimen samples may contain more or less IgY and will need to be diluted appropriately. A 10-fold dilution is usually sufficient to avoid possible matrix interference.

### TEST PROCEDURE

Allow all reagents to reach room temperature before use. Prepare reagents as described above. Label test tubes to be used for the preparation of standards and specimen samples. If the entire microplate will not be used for testing, remove surplus strips from the plate frame and place into the sealable plastic bag with desiccant. Seal bag and store at 2-8°C.

**Step 1:** Label each strip on its end tab to ensure identity should the strips become detached from the plate frame during the assay.

**Step 2:** Pipette 200  $\mu$ l of standards 1-6 into duplicate wells.



**Step 3:** Pipette 200  $\mu$ l of each specimen sample into duplicate wells.

**Step 4:** Cover the microplate with a plate sealer and incubate for 30 minutes at room temperature (18-25°C).

**Step 5:** Aspirate the contents of each well and wash 4 times with 1X Plate Wash Buffer (See Preparation of Reagents section). To wash, fill the wells with at least 300  $\mu$ l of 1X plate wash buffer and aspirate. Perform 4 fill/aspirate cycles. After the final wash cycle, thoroughly blot the plate by carefully striking on a pad of absorbent paper towels. Continue striking until no visible droplets of Plate Wash Buffer are observed.

**Step 6:** Pipette 100  $\mu$ l of Chicken IgY Detector Antibody into each well.

This product was manufactured in a facility which has a Quality Management System that is ISO 13485 certified.

REF	Catalog Number		Temperature Limitation
LOT	Lot Number		Expiration Date
RUO	For Research Use Only		

ZeptoMetrix Corporation  
878 Main Street  
Buffalo, NY 14202  
800-274-5487  
www.zeptometrix.com

## Chicken IgY (IgG) ELISA

Catalog Number: 0801010

**Step 7:** Cover the plate with a plate sealer and incubate for 30 minutes at room temperature (18-25°C).

**Step 8:** Wash the plate 4 times with 1X Plate Wash Buffer as described in Step 5.

**Step 9:** Pipette 100 µl of Substrate into each well.

**Step 10:** Incubate the plate for 30 minutes at room temperature (18-25°C) without a plate cover. A blue color will develop in wells containing chicken IgY.

**Step 11:** Pipette 100 µl of Stop Solution into each well. A color change from blue to yellow will occur. Gently tap microplate to mix.



**Step 12:** Within 15 minutes, read the optical density of each well at 450 nm using a microplate reader.

### EXPECTED RESULTS

Below is an example of a standard curve and should not be used to calculate actual samples. Variations may be observed from laboratory to laboratory due to pipetting, incubator temperatures, plate readers, etc.

Chicken IgY Standard Concentration	Optical Density at 450 nm
125 ng/ml	1.838
62.5 ng/ml	1.146
31.25 ng/ml	0.734
15.6 ng/ml	0.437
7.8 ng/ml	0.265
0 ng/ml	0.065


This product was manufactured in a facility which has a Quality Management System that is ISO 13485 certified.

REF	Catalog Number		Temperature Limitation
LOT	Lot Number		Expiration Date
RUO	For Research Use Only		

**ZeptoMetrix Corporation**  
 878 Main Street  
 Buffalo, NY 14202  
 800-274-5487  
[www.zeptometrix.com](http://www.zeptometrix.com)

## Chicken IgY (IgG) ELISA

Catalog Number: 0801010

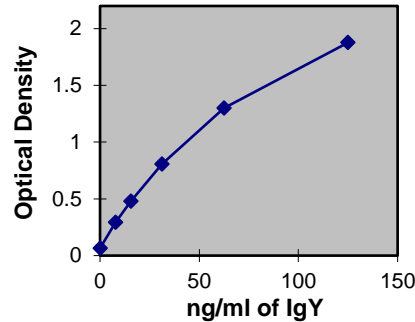

### CALCULATION OF RESULTS

#### Test Validity:

- The mean optical density of the 0 ng/ml standard must be below 0.200.
- The mean optical density of the 125 ng/ml must be above 1.000.
- It is recommended that specimen samples be re-assayed with a greater or lesser dilution when the mean optical density value does not fall within the standard curve.

#### Calculation:

1. Calculate the mean optical density (OD) values for each set of standards and diluted specimen samples.
2. Using linear graph paper or graphing software, plot the mean OD values of each standard on the Y-axis versus the corresponding concentration of standards on the X-axis.
3. Draw the best fit curve through these points to construct a standard curve. A point-to-point construction will be the most accurate.
4. Determine the IgY concentration of each diluted specimen sample by interpolation from the standard curve.
5. Multiply by the dilution factor used to dilute each specimen sample to determine the IgY concentration of the original specimen sample.



### PERFORMANCE CHARACTERISTICS

#### Specificity:

The chicken IgY detector antibody in this kit has been shown by immunoelectrophoresis and/or ELISA to react only with the Fc portion of the Chicken IgY heavy chain but not with the Fab portion of chicken immunoglobulins. No reactions to other non-immunoglobulin serum proteins were detected.

Serum from sheep, rabbit, rat, donkey, goat, horse, bovine, mouse and human had no reaction with this ELISA test.

This product was manufactured in a facility which has a Quality Management System that is ISO 13485 certified.

REF	Catalog Number		Temperature Limitation
LOT	Lot Number		Expiration Date
RUO	For Research Use Only		

**ZeptoMetrix Corporation**  
 878 Main Street  
 Buffalo, NY 14202  
 800-274-5487  
 www.zeptometrix.com



## Chicken IgY (IgG) ELISA

Catalog Number: 0801010

**Precision:**

Sample	IgY ng/ml	Intra-assay %CV (n=16)	Inter-assay %CV (n=48)
High Sample	113	4%	7%
Medium Sample	25	3%	5%
Low Sample	6	7%	10%

This product was manufactured in a facility which has a Quality Management System that is ISO 13485 certified.


REF	Catalog Number		Temperature Limitation
LOT	Lot Number		Expiration Date
RUO	For Research Use Only		

**ZeptoMetrix Corporation**  
 878 Main Street  
 Buffalo, NY 14202  
 800-274-5487  
[www.zeptometrix.com](http://www.zeptometrix.com)



## Chicken IgY (IgG) ELISA

Catalog Number: 0801010
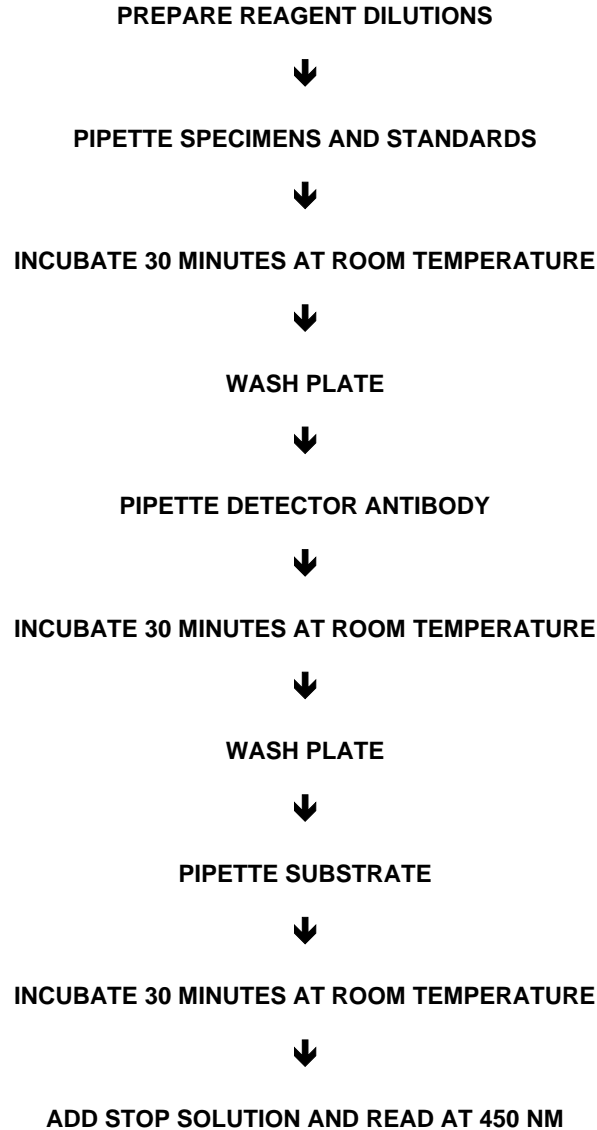
### PROCEDURAL FLOW CHART



This product was manufactured in a facility which has a Quality Management System that is ISO 13485 certified.

REF	Catalog Number		Temperature Limitation
LOT	Lot Number		Expiration Date
RUO	For Research Use Only		

ZeptoMetrix Corporation  
 878 Main Street  
 Buffalo, NY 14202  
 800-274-5487  
[www.zeptometrix.com](http://www.zeptometrix.com)